

FIG. 1

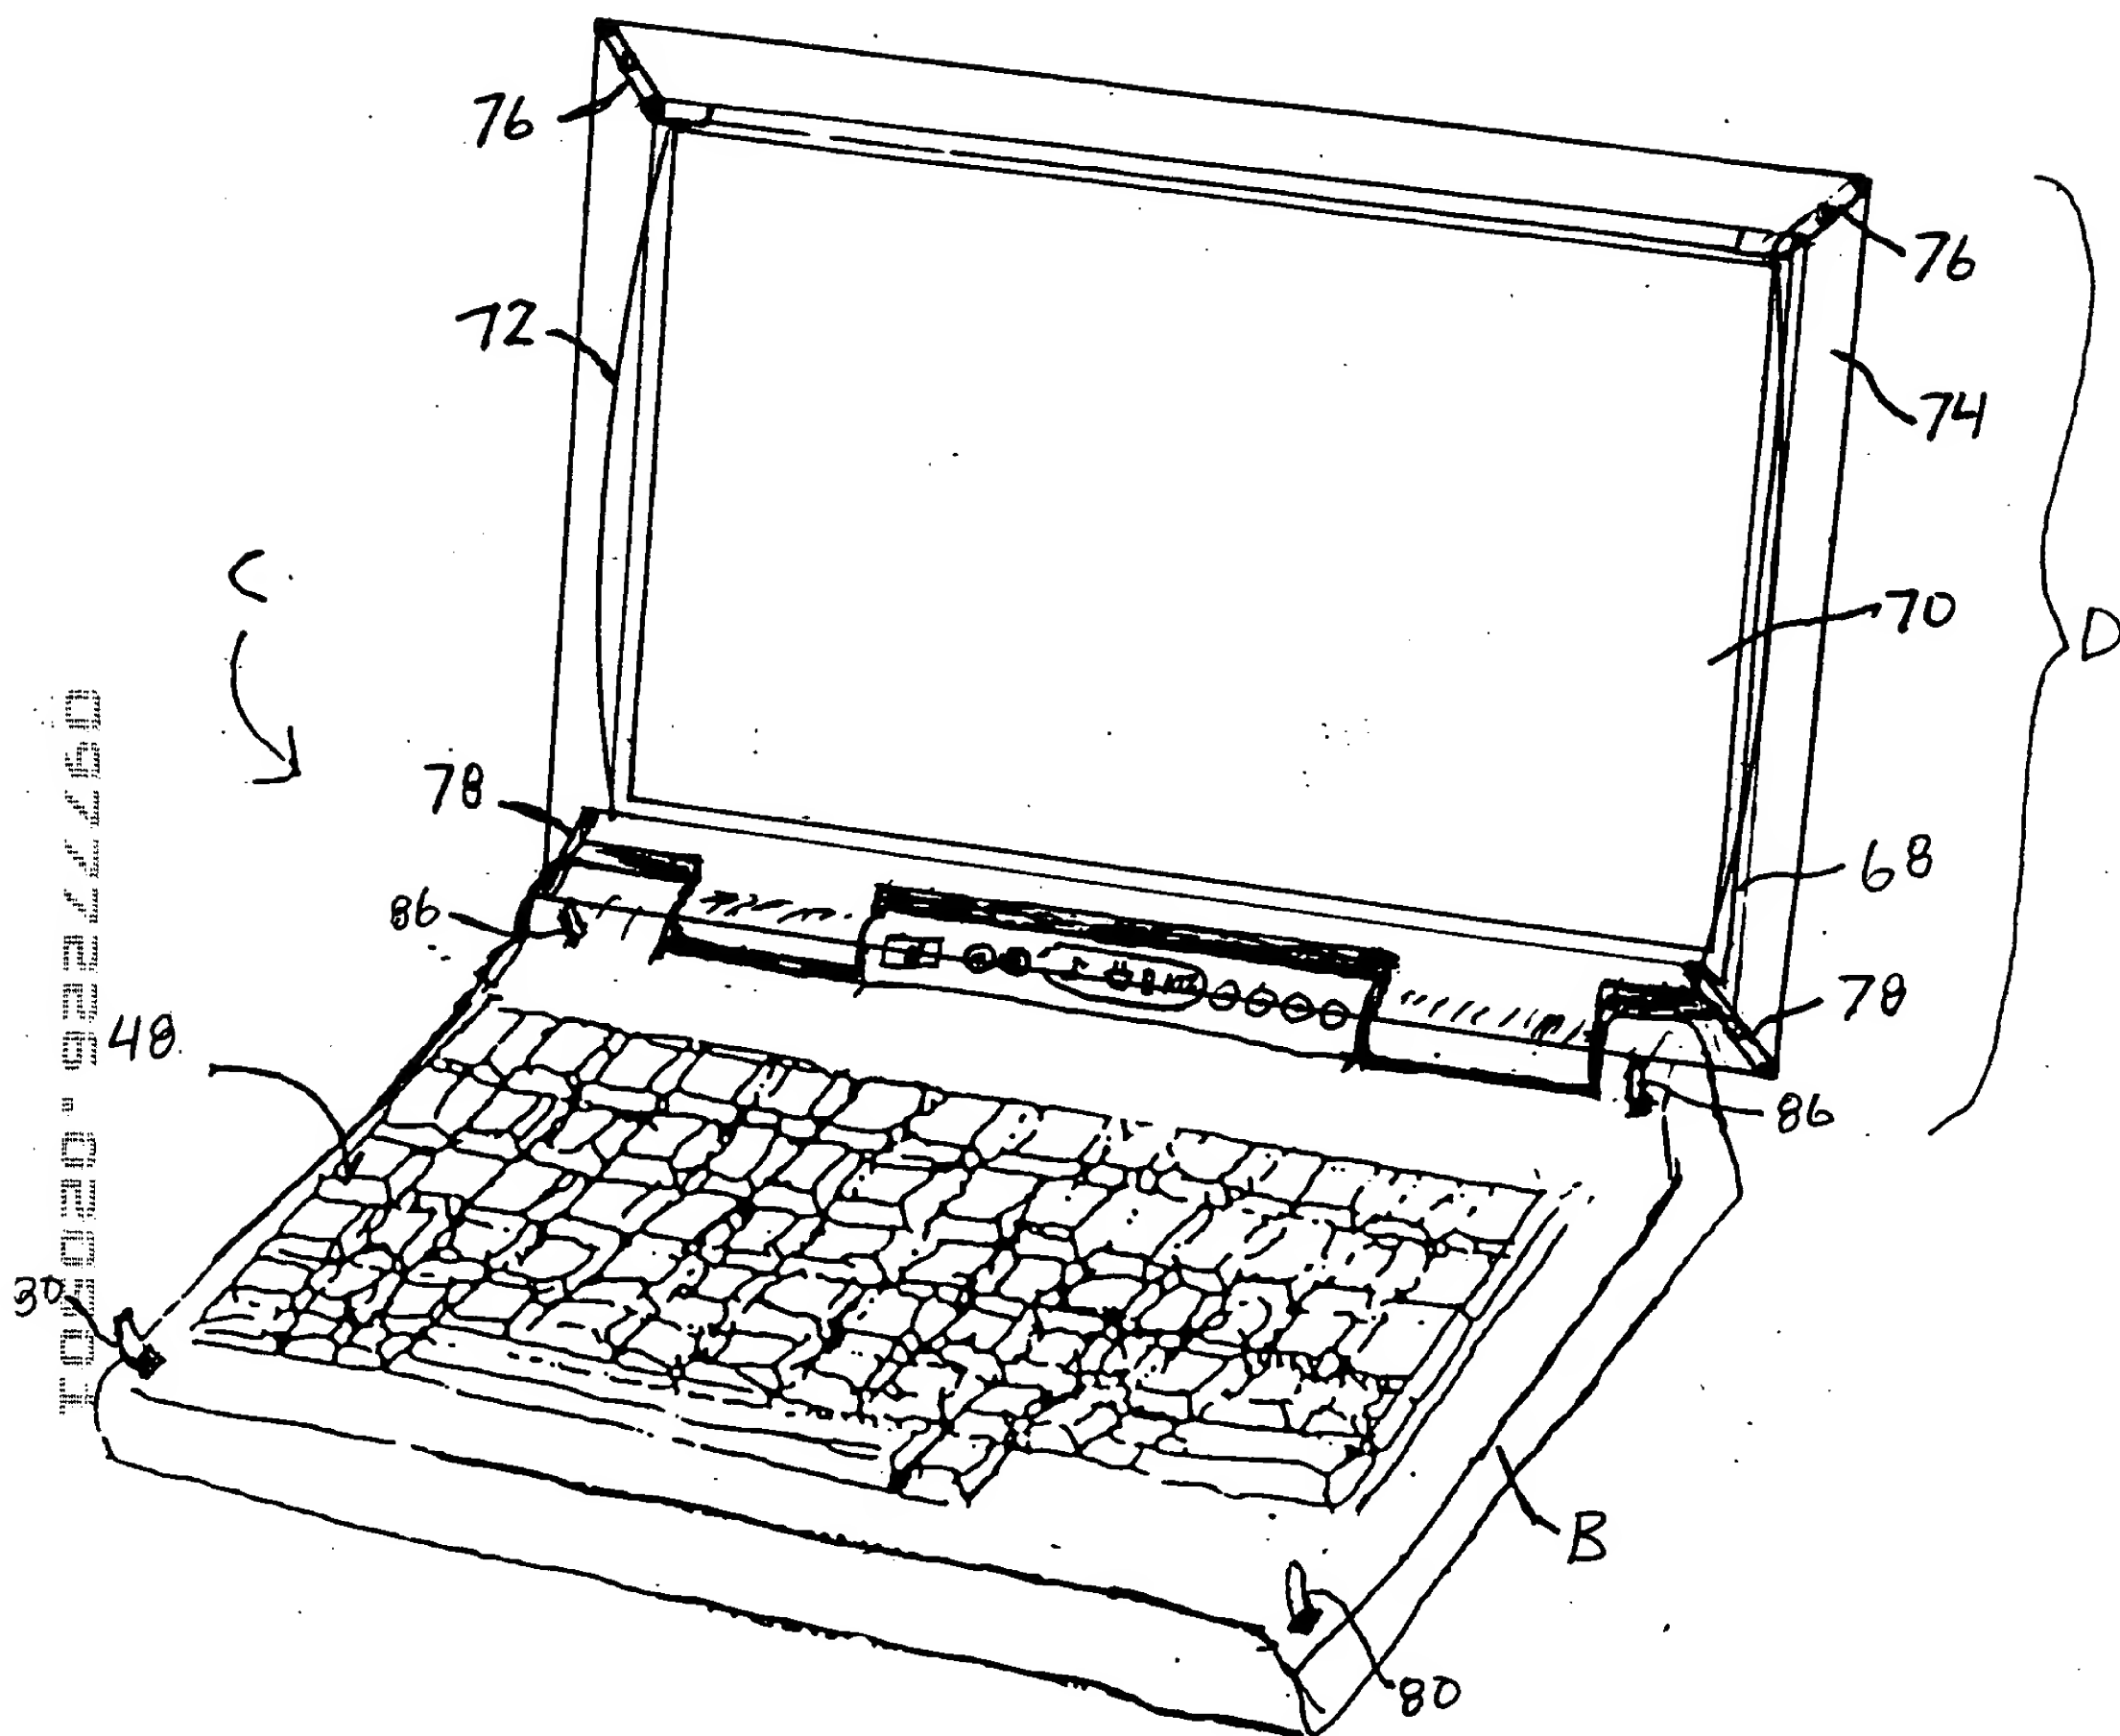


FIG. 2

FIG. 3 is a cross-sectional view of the device.

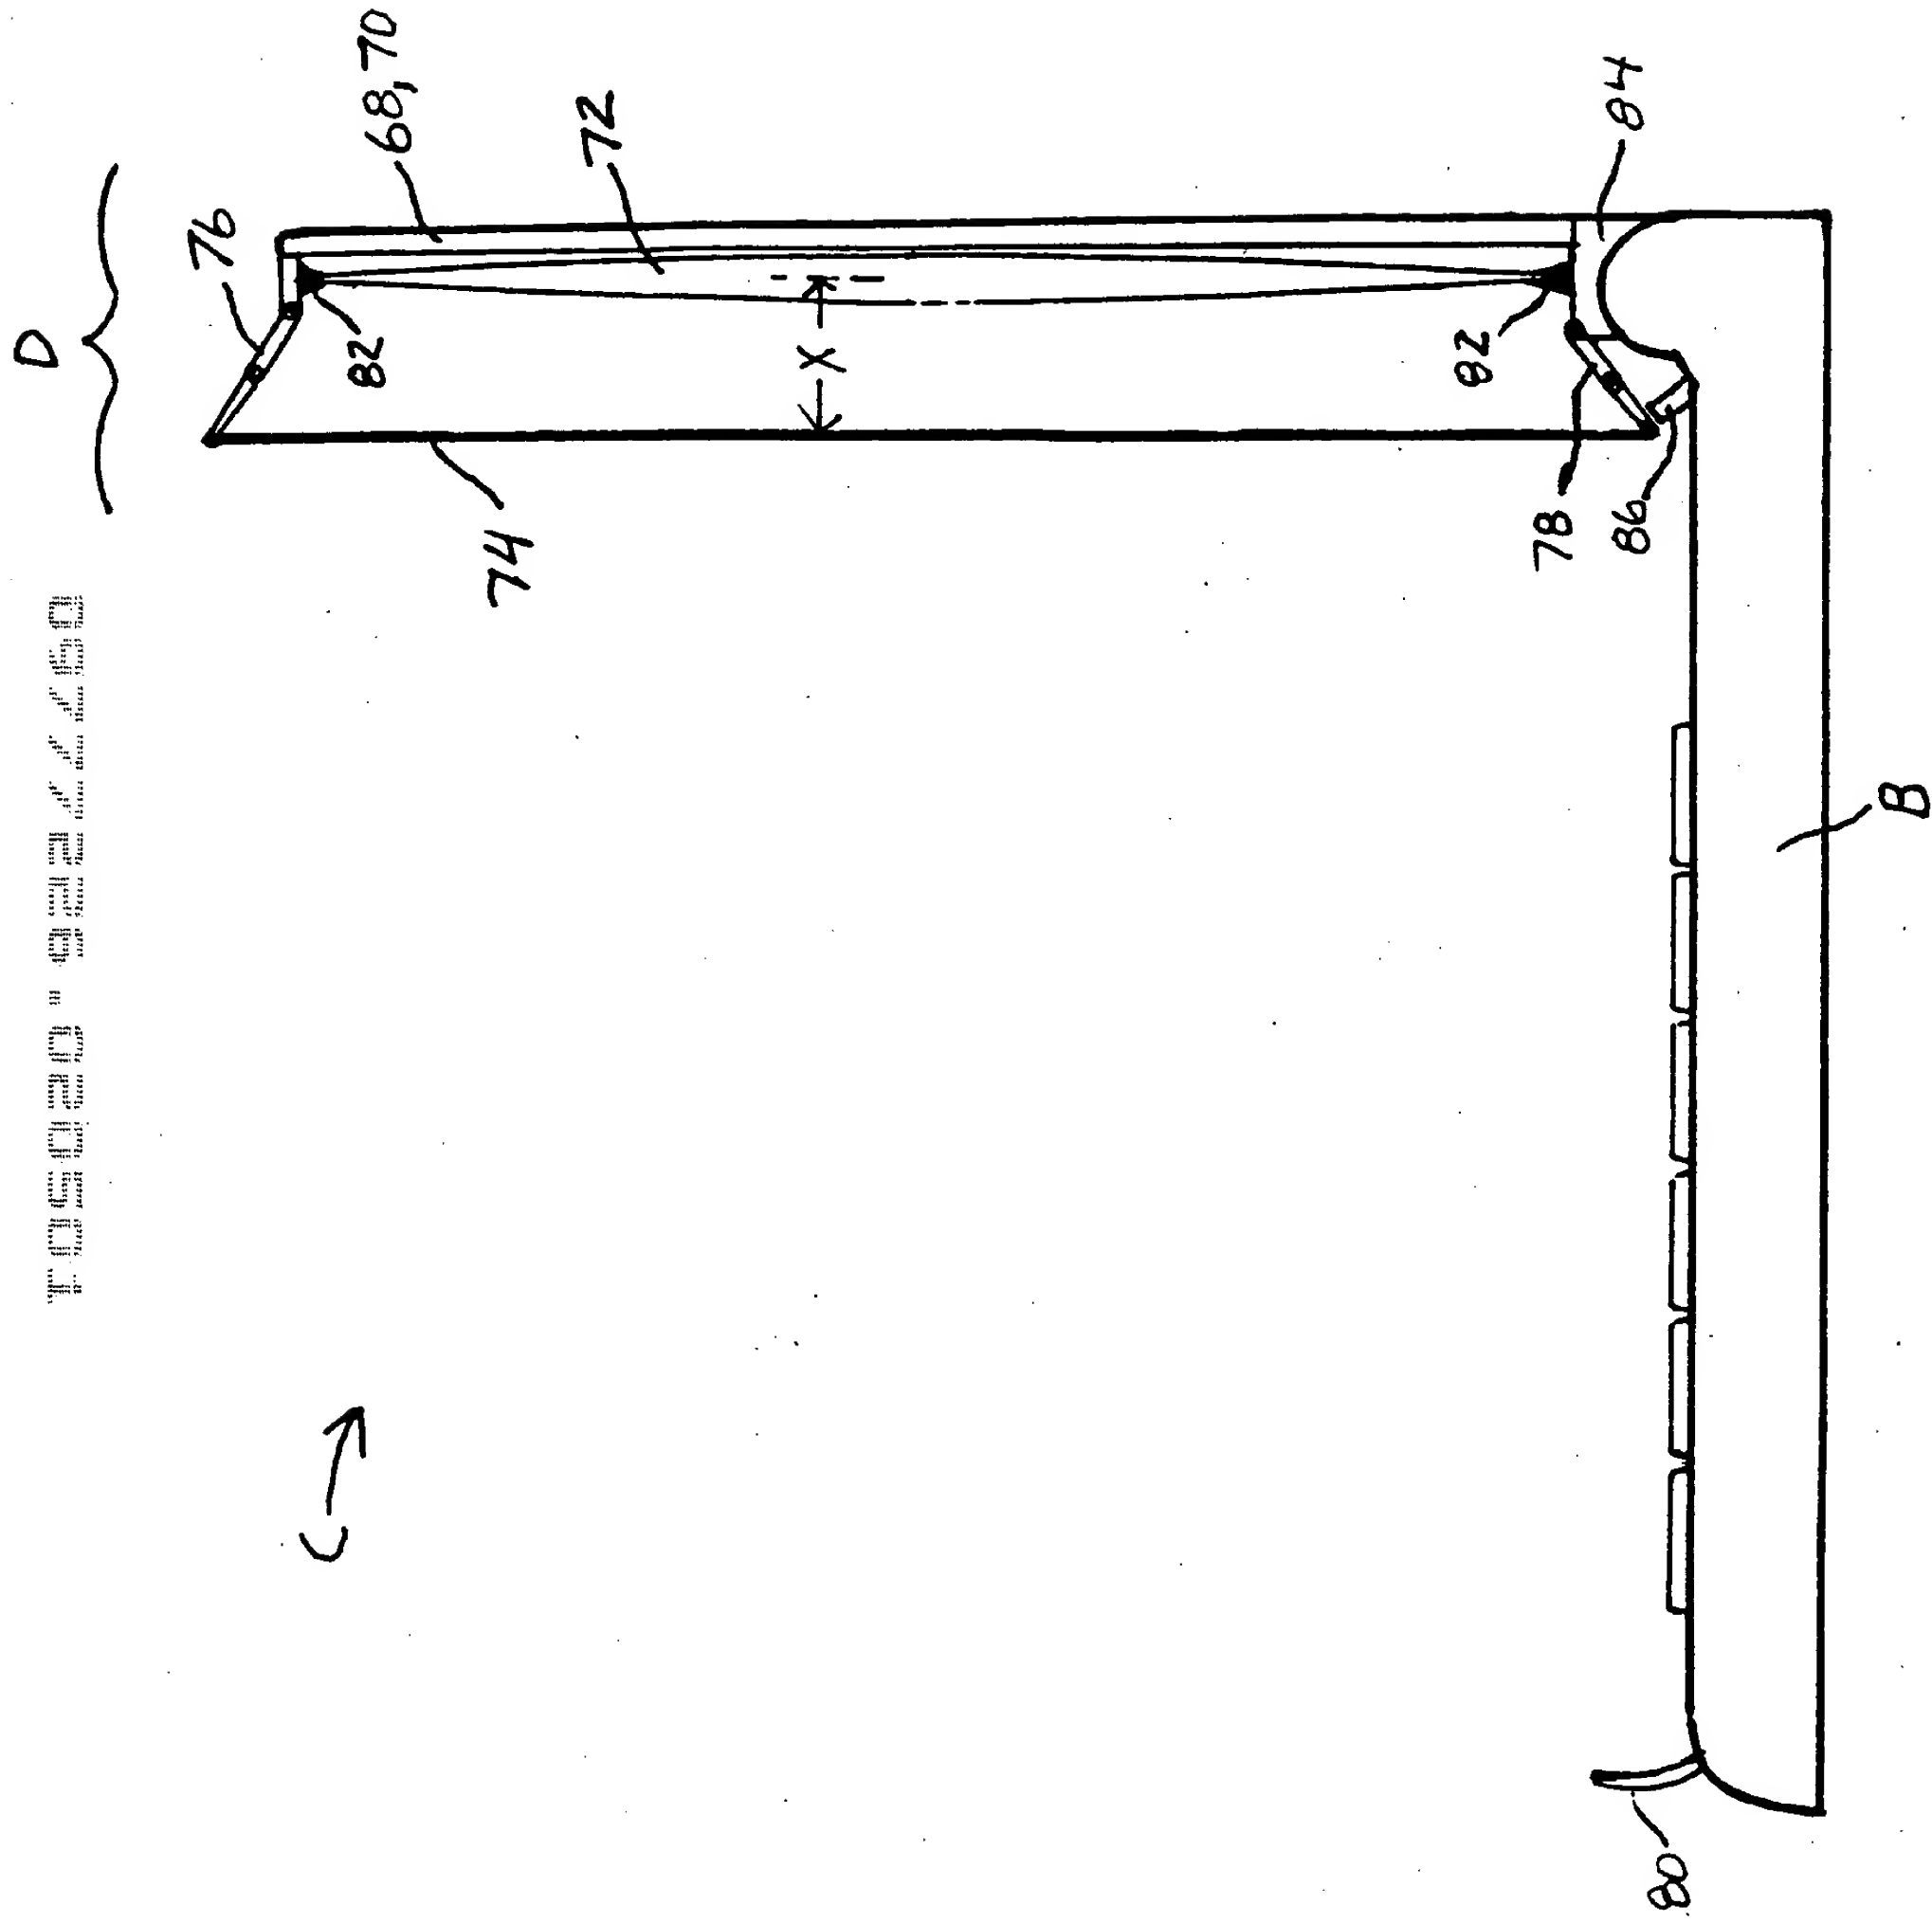


FIG. 4

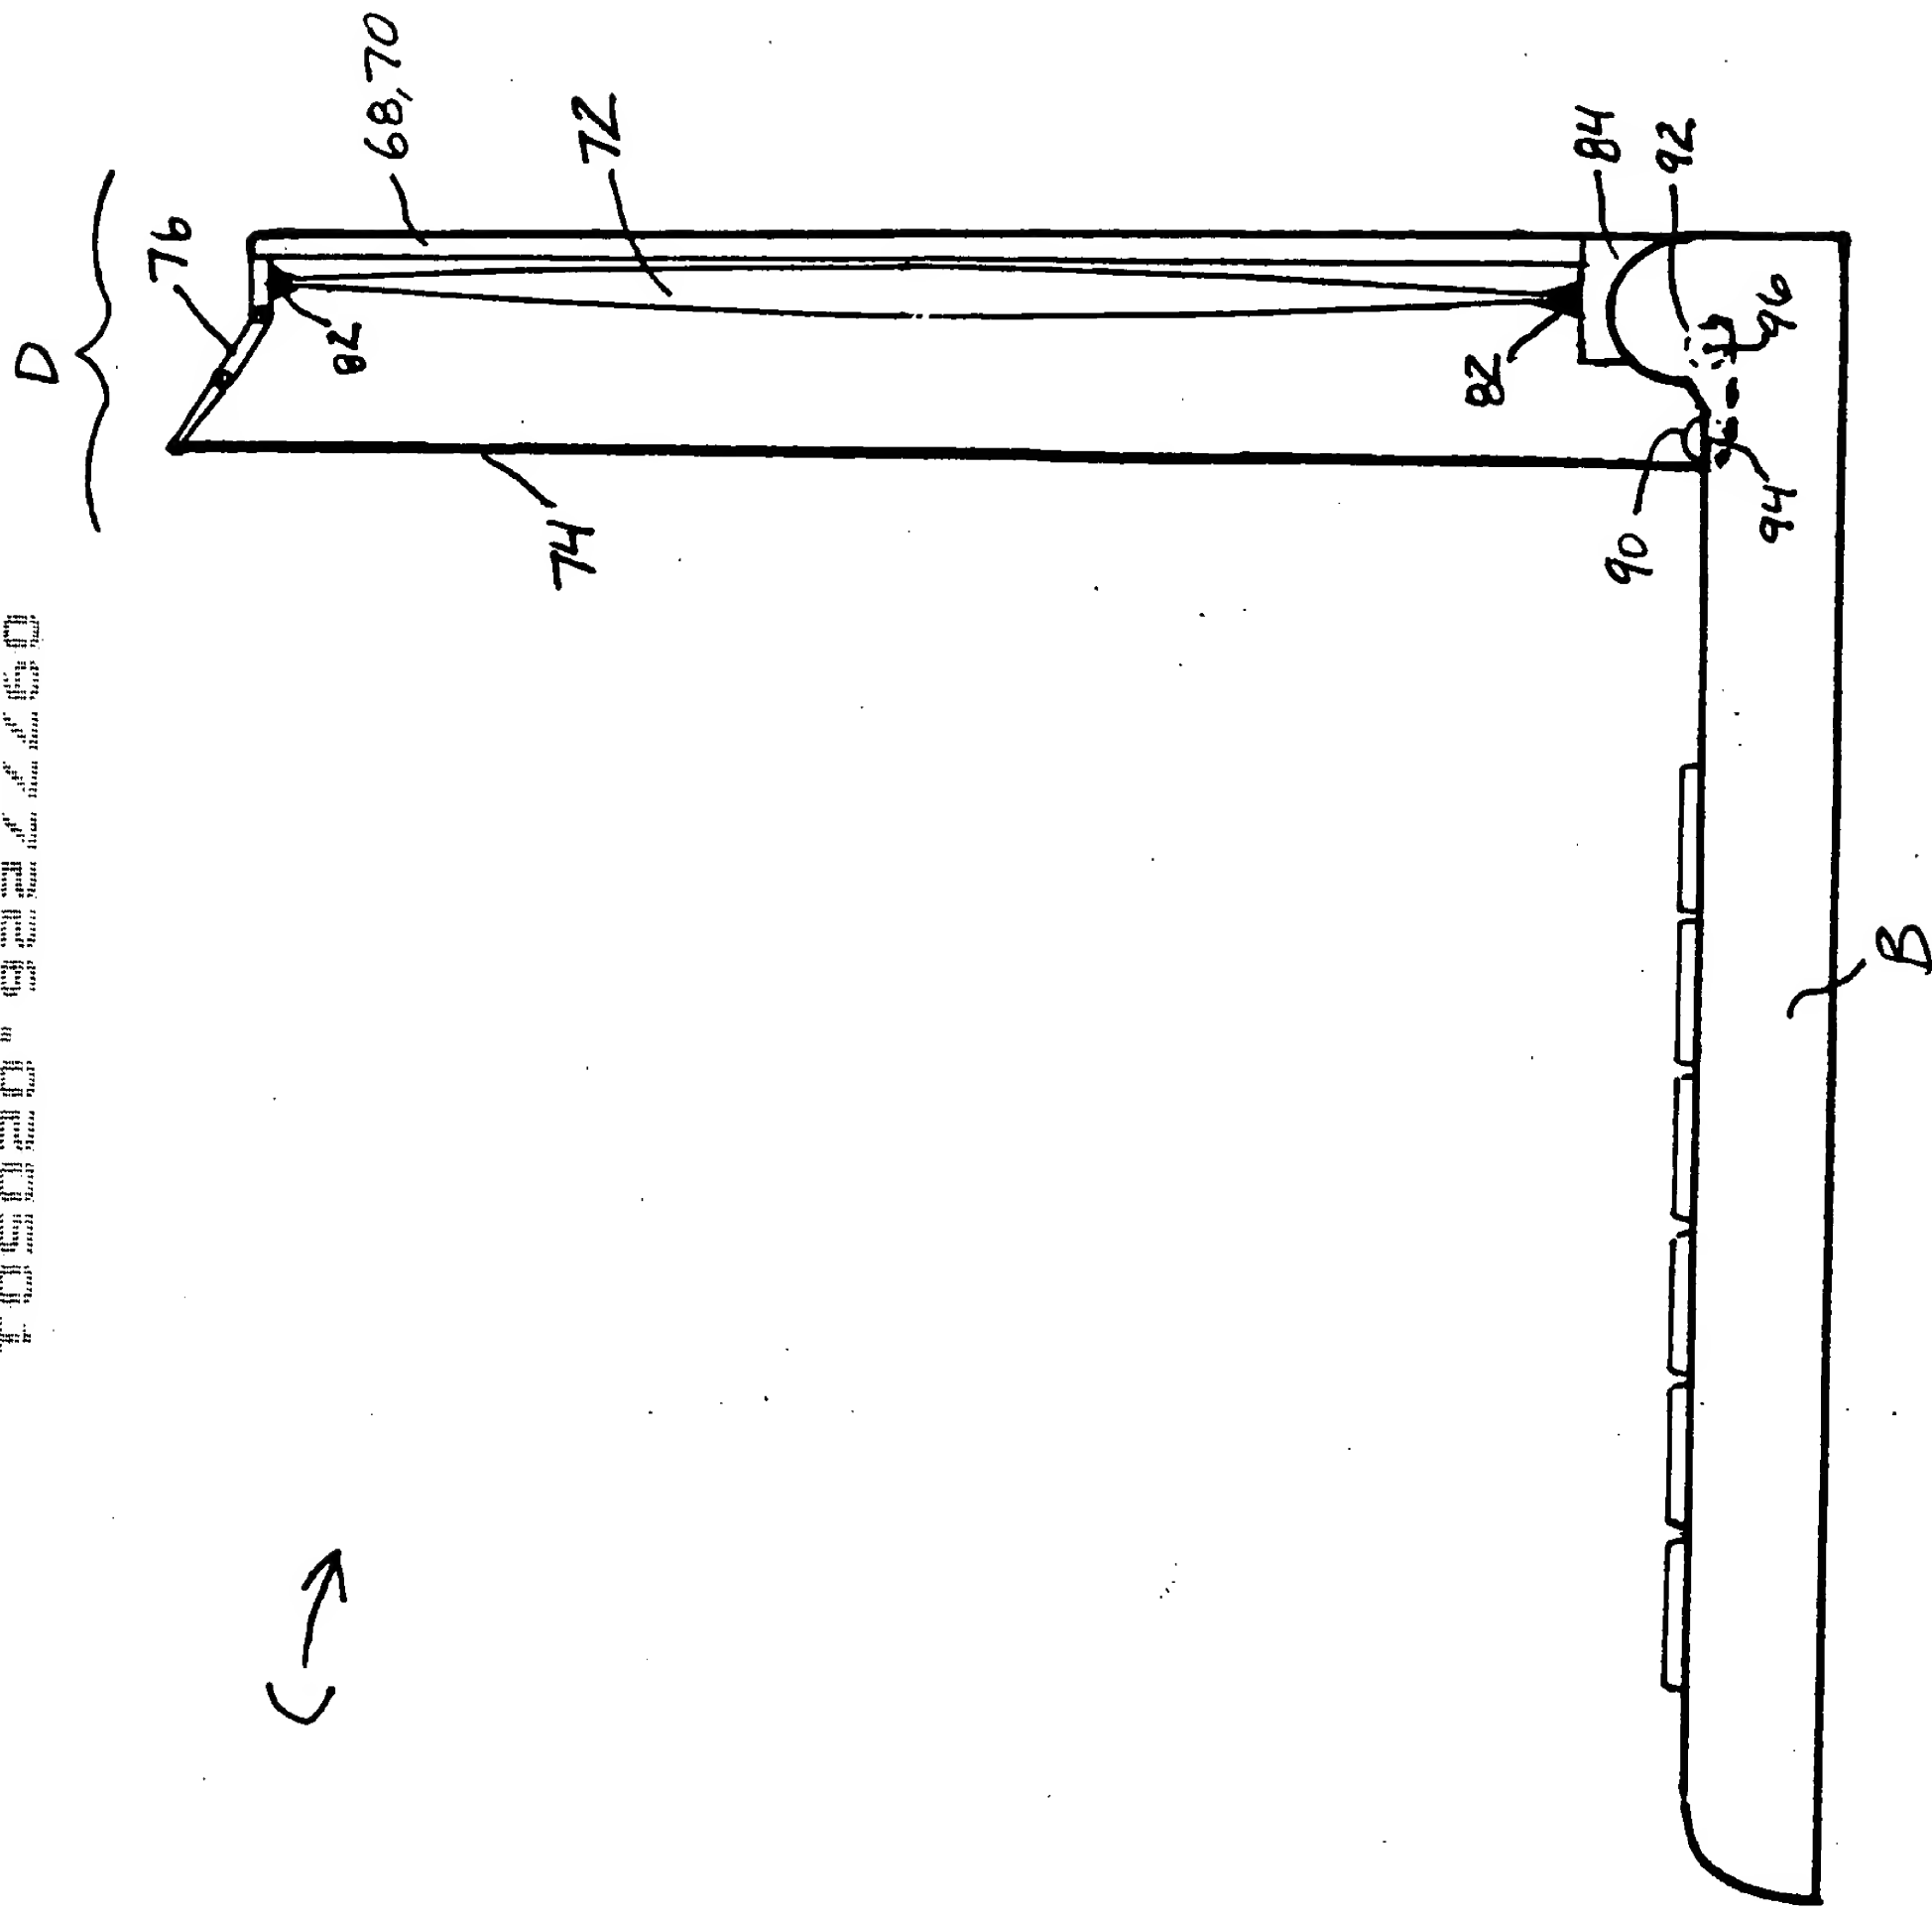



FIG. 4

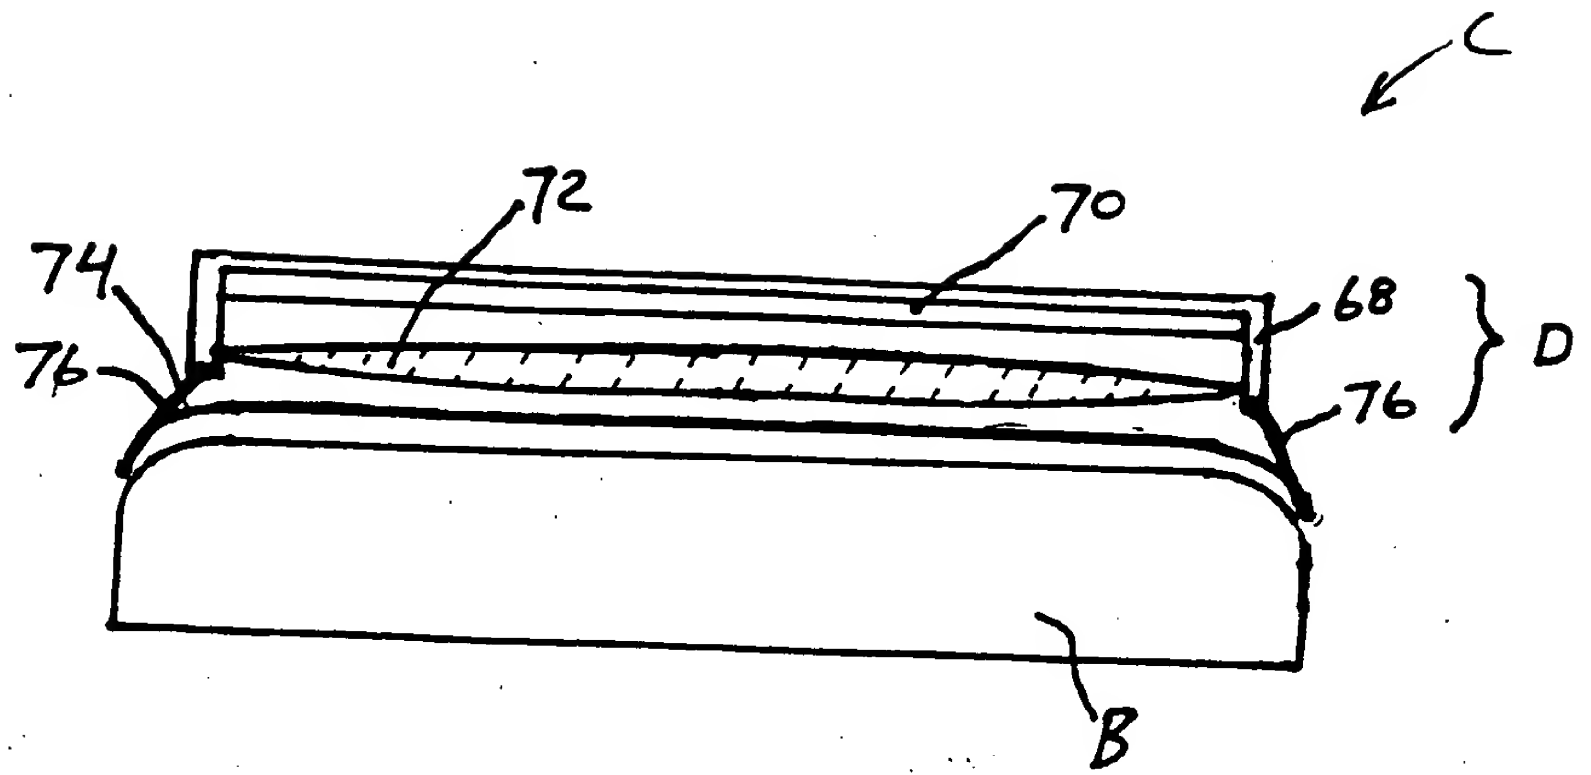


FIG. 5

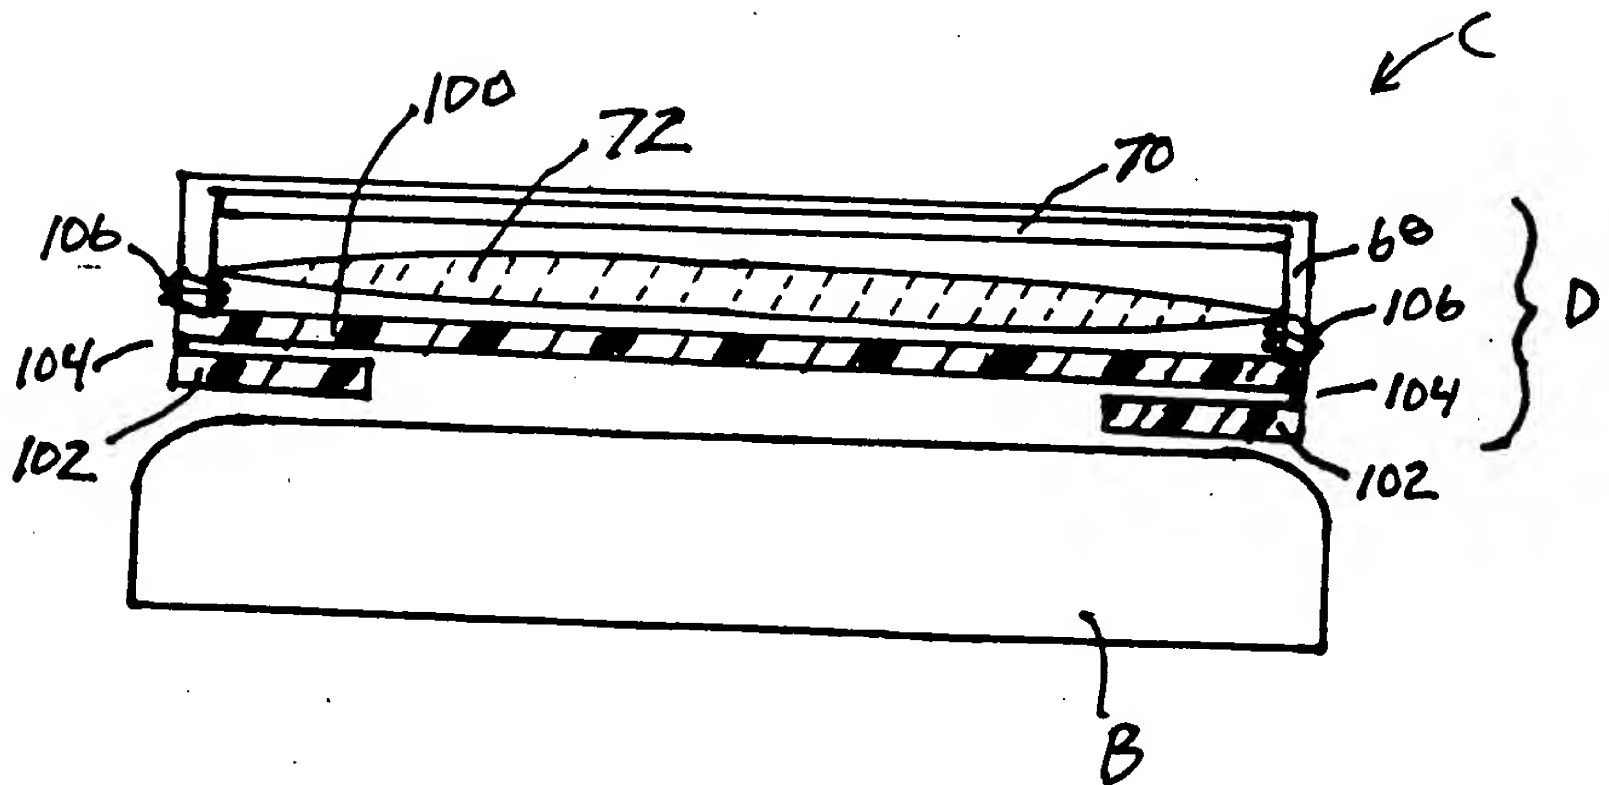


FIG. 6